



+ Pekkton® ivory –
Instructions for use.

Pressing technique with Dekema.

Made with
{Pekkton}®

	Page
1 Product name	3
2 Product description	3
3 General information	3
3.1 Intended use	3
3.2 Disposal	3
4 Instructions for use	3
4.1 Indications	3
4.2 Contraindications	3
4.3 Warnings	3
4.4 Preventive measures	3
4.5 Side effects	3
5 Instructions for use	4
5.1 Preparation	4
5.2 Framework criteria	4
5.3 Model and stump preparation	5
5.4 Production in the pressing process	5
5.4.1 Pressing device	5
5.4.2 Waxing	5
5.4.3 Sprueing	6
5.4.4 Investing	6
5.4.5 Preheating	8
5.4.6 Pressing	9
5.4.7 Divestment and cleaning	10
5.5 Conditioning	11
5.6 Veneering	12
5.6.1 Preparation	12
5.6.2 Veneering concepts	12
5.7 Bond to titanium bases (laboratory)	12
5.8 Try-in and cementation	13
5.8.1 Disinfection	13
5.8.2 Cementation	13
5.9 Handling after integration	13
5.9.1 Cleaning and follow-up	13
5.9.2 Traceability	13
6 Ordering information	14
7 Symbols	15
8 Disclaimer / Validity	15
9 Availability	15
10 Copyright and trademarks	15
11 Further information	16
11.1 Troubleshooting	16
11.2 FAQ's	17

Rx only

Medical devices of Cendres+Métaux SA correspond to the Medical Device Directive 93/42/EEC and carry the CE mark. See packaging for details.

1 Product name

Pekkton® ivory (pressing blanks)


2 Product description


Pekkton® ivory is a high performance material (based on PEKK) composed of OXPEKK® IG¹ (Implantable Grade with highest purity) and Oxide for optimization of tint and mechanical properties. Color: whitish.

The material is available to users, among other things, as a pressing blank. The dental technician fabricates crown and bridge frameworks from the pressing blank. The frameworks are then esthetically veneered in the laboratory with bonded pressable crowns, veneering composites, prefabricated acrylic teeth or trays.

3 General information

For the exact specifications of Pekkton® ivory, please refer to the material data sheet and the safety data sheet. You will find the data sheets mentioned free of charge at www.pekkton.com.

 Important information for the specialist / note instructions for use.


 Warning symbol for increased caution.

3.1 Intended use

Pekkton® ivory is intended to be used for long-term, temporary dental crowns and bridge frameworks.

3.2 Disposal

Pekkton® waste can be disposed of along with normal household garbage.

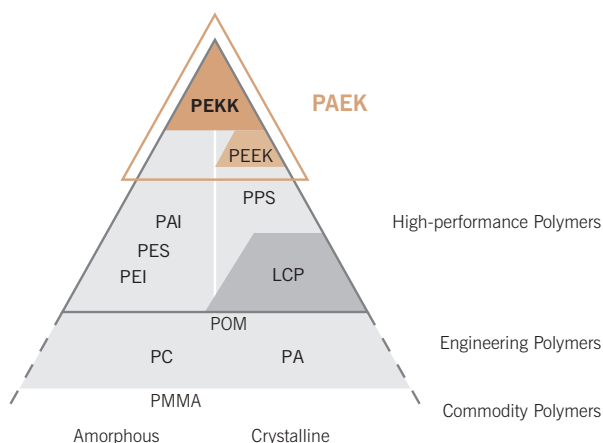


4 Instructions for use

4.1 Indications

(Pekkton® ivory)

- Long-term, temporary veneered single crowns and 3-unit bridges in the frontal and side region for a maximum wearing time of 12 months.
- Long-term, temporary unveneered crowns in the side region for a maximum wearing period of 12 months
- Unveneered parts e.g. crown margins and backings.

 The responsibility for the use of custom-made products beyond the described indications lies with the dentist.

4.2 Contraindications

(Pekkton® ivory)

- Bridge reconstructions with more than one intermediate element.
- Patients with parafunctions e.g. bruxism.
- Unveneered crowns in the lateral mouth area for use of more than 12 months.
- Veneered single crown and 3-unit bridge in the frontal and side mouth area for a use exceeding 12 months.
- Crowns and bridges with less than 1.3 mm of occlusal space.
- When the minimum dimensions of the framework cannot be maintained:
 - Minimum circular wall thickness less than 0.6 mm
 - Minimum occlusal wall thickness less than 0.8 mm
 - Connector dimensions of front (anterior) bridges less than 10 mm²
 - Connector dimensions of side (posterior) bridges less than 12 mm²
- When patients have a known allergy to one or more components of the material.

4.3 Warnings

If patients are allergic to one or more elements of the material, the latter should not be used. In patients with suspected allergy to one or more elements of the materials, this product may only be used following allergological clarification and proof of non-existence of an allergy.

Pekkton® ivory has not been evaluated for safety and compatibility in the MR environment. Pekkton® ivory has not been tested for heating or migration in the MR environment.

For further information, please contact your Cendres+Métaux representative.

4.4 Preventive measures

When grinding the Pekkton® framework, wear protective goggles with a dust mask and use a suction unit.


4.5 Side effects

No known side effects if used as intended.

¹ Pekkton® based on OXPEKK® from OPM, Oxford Performance Materials, USA.


5 Instructions for use

5.1 Preparation


 A reduction in framework thickness always means a reduction in strength. This aspect must be considered in the preparation, in particular within the occlusal area. The height of the crown die preparation should be at least 4 mm and the angle of convergence should be 4–6°. Eliminate undercuts.

Principally, the preparation technology corresponds to the one of full ceramic reconstructions.


The preparation is based on the concept of reduced, anatomical form. A chamfer preparation in the angle of approx. 10–30° or a shoulder preparation with rounded inside edges is ideal. The width of the chamfer/shoulder is approx. 0.8 mm.

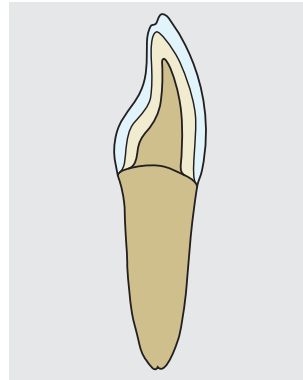

Preparation design of a anterior tooth

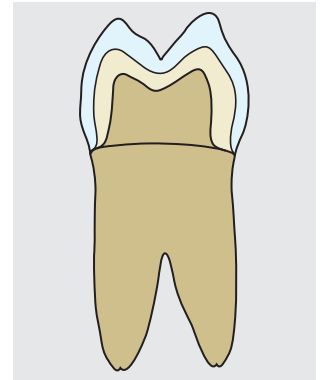


Preparation design of a molar

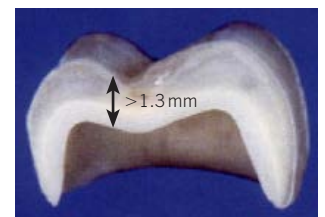


Minimal occlusal thickness


5.2 Framework criteria

 The key for clinical success and a durable restoration in the patient's mouth is compliance with the guidelines for the design of a crown or bridge in Pekkton®. The change from framework to veneering material may not occur in the functional contact area. In there is a lack of space, please respect the maximal possible framework thickness. For an optimal color reproduction, a veneering thickness of 0.5 mm is recommended. The occlusal minimum thickness of a crown should be < 1.3 mm.

Material thickness of the frameworks

Pekkton® ivory	Crown		Bridge	
	Anterior tooth	Posterior tooth	Anterior tooth	Posterior tooth
Design type	Tooth shape-supporting	Cusp supporting	Tooth shape-supporting	Cusp supporting
Minimum wall thickness circular	> 0.6 mm	> 0.6 mm	> 0.6 mm	> 0.6 mm
Minimum wall thickness occlusal	> 0.8 mm	> 0.8 mm	> 0.8 mm	> 0.8 mm
Connector dimensions	–	–	> 12 mm ²	> 14 mm ²

 The stability of the connector surface is increased when the ratio of vertical to horizontal is significantly greater (ratio of approx. 60% to 40%).

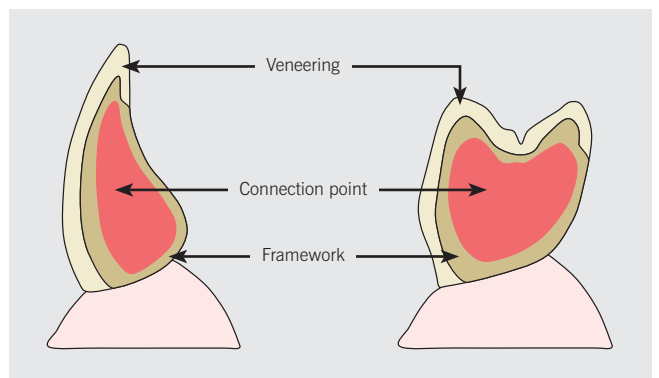


5.3 Model and stump preparation

Careful preparation of the work models is required to obtain a well fitting crown or bridge.

The dies must fit reproducibly and be removable.

It is advisable to apply a sealer to harden the surface and to protect the die.

Two layers of spacer are applied to maximum 1mm from the preparation margin.

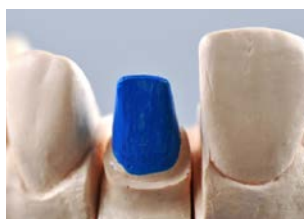

Anterior tooth



Posterior tooth

5.4 Production in the pressing process

5.4.1 Pressing device

4 Recommended pressing devices for processing Pekkton® ivory. To make sure the material is homogeneous, it must be possible to cool Pekkton® ivory under pressure after the pressing operation. The following devices meet this requirement:

AUSTROMAT 654 press-i-dent


AUSTROMAT 3001 press-i-dent

Manufacturer:

DEKEMA Dental-Keramiköfen GmbH, D-83395 Freilassing
(This product is marketed by the DEKEMA company and DEKEMA applies the CE mark.)



5.4.2 Waxing


 Only use wax that can be burned out without leaving a residue.

Design the caps and bridge elements in accordance with the basic principle of the maximum possible framework thickness, as well as the cusps-supported reduced tooth form.


Avoid dirt-collecting recesses on the gingival design when modeling the pontics.

A thin garland can be designed circularly or partially on the posterior tooth.

In case of insufficient space, a direct stop can also be prepared.

 For larger bridge work, form the palatal / lingual part in the framework material Pekkton® ivory in favor of a maximum possible framework thickness and do not veneer.

Posterior tooth (molar)

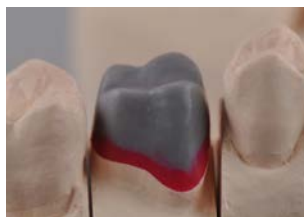

Buccal



Palatal/lingual

Anterior tooth



Labial circular tapered edge design



Palatal/lingual mini edge (garland)



Buccal/labial



Palatal/lingual




After pressing. Conditioned on the model.



Finished and polished Pekkton® ivory bridge.

5.4.3 Sprueing


The sprues should be attached in an angle of 5–10°, similar to the indications for press ceramic systems.

 It is essential to avoid sharp edges because when pressing viscous Pekkton® investment material can be entrained. This can prevent inclusions, especially in the marginal zone. Respect the length of the press channel to avoid loss of pressure.



	Single tooth crown	Bridge
Press channel	Diameter 12 mm	Diameter 12 mm
Ring system recommendation	Investment ring system Empress (Ivoclar Vivadent, FL-Schaan)	Trixpress (Dekema)
Size of the investment ring	100 g (suitable for 1 or a maximum of 2 equal-sized items) 200 g (suitable for 4 items max.)	200 g (suitable for 4 items max.) 380 g (suitable for up to complete bridges)
Diameter of the wax wire	3 to 3.5 mm	3 to 3.5 mm
Length of press channel (wax wire)	3 to 5 mm (max. height incl. object 18 mm)	3 to 5 mm (max. height incl. object 18 mm)
Sprue point at the object	Aligned with the die (prevents it from breaking off)	Fit the press channel to the connection point.
Sprue angle to the object	axial	axial
Sprue angle to investment ring base	In a small angle of approx. 5–10°	In a small angle of approx. 5–10°
Design of sprueing points	trumpet shape, without sharp edges and angles	trumpet shape, without sharp edges and angles
Distance between various objects	> 3–5 mm	> 3–5 mm
Distance to margin of investment ring	10 mm	10 mm
Air outlets	Not necessary	For larger bridge elements, fit air outlets (∅ 0.8–1 mm) to reduce pressure and to avoid bubbles.

5.4.4 Investing

 Please weigh the wax object including the pressing channel to avoid pressing with too little material. Do not use a debubblizer on the wax objects e.g. spray (danger of micro bubbling on the surface).

	Weight	Indication
Investment ring	100g	Wax weight max. 1.2 g Maximum 2 single crowns of small to medium size.
Investment ring	200g	Wax weight of 1.2g max. per press channel From 1 to a max. 4 single crowns of each size per press channel*.
Investment ring	380g	Wax weight of 1.2g max. per press channel From 1 to a max. 4 single crowns of each size per press channel (use max. 5 press channels for large objects)*.

* With the investment ring former set from DEKEMA, it is possible to use more than one press channel.

Please follow the manufacturer's work instructions.

Definition of wax weight:


1. Put the base of investment ring without wax objects on the balance and calibrate to 0.
2. Fix the wax objects on the base of the investment ring.
3. Put the base of investment ring with the wax objects on the balance.
4. The indicated value corresponds to the wax weight.

Recommended investment volumes		Manufacturer		
Standard process:	CM-20	Cendres + Métaux SA, CH-Biel/Bienne		
Speed process:	AnaxVest pm	Anaxdent, DE-Stuttgart		
	IPS PressVEST Speed	Ivoclar Vivadent, FL-Schaan		

	Mixing ratio	CM-20 Liquid	Dist. water	Total
CM-20	100 g	19 ml	6 ml	25 ml
	200 g	38 ml	12 ml	50 ml

	Mixing ratio	Liquid	Dist. water	Total
AnaxVest pm	100 g	18 ml	6 ml	24 ml

	Object	Liquid	Dist. water
IPS PressVEST Speed	Crown	60 %	40 %
	Bridge	50 %	50 %

 Please follow the manufacturer's instructions for use for correct processing of the investment material!
Other investment materials are not recommended because the bond between Pekkton® and the quartz particles in the investment material is often too strong.

Slowly and carefully fill in the investment material up to the wax margin.



Use a suitable instrument for the fine investment of the cavity (e.g. small brush), so that the humidity will not be withdrawn from the investment material.




A fine probe can also be used. Please make sure that the delicate wax margins are not damaged.

Carefully fill the investment ring up to the margin and position the ring gauge with a combined hinged and rotating movement.




- Allow the investment ring to set without vibration.
- No hardening under pressure (e.g. in a pressure pot)
- No investing before a weekend
(Danger of drying out or too much humidity through Hygrophor)


5.4.5 Preheating

 Check temperature precision of the burnout furnace regularly.
Please follow the manufacturer's work instructions.


After setting of the investment material according to manufacturer' indications, the investment ring is prepared for preheating.


1. Carefully turn and remove the investment gauge.
2. Carefully turn and remove the investment ring base, too.
3. Remove rough spots with a plaster knife or a belt grinder.
4. Please make sure that no investment material enters the press channel.

 The investment ring base should have a 90° angle and be situated flat on the investment ring holder in the pressing furnace.

	Standard	Speed	
	CM-20	AnaxVest pm	IPS PressVEST Speed
Setting time	30 minutes	30–35 minutes	30–45 minutes
Program (preheating furnace)	Stand-by temperature: room temperature Rate of rise: 5 °C/min. Phase 1: 250 °C for 60 min. Phase 2: 800 °C for 60 min. Phase 3: Cooling in the furnace at 390 °C	Stand-by temperature: 650 °C Burn out and preheating: 60 min. at 650 °C	Stand-by temperature: 850 °C Burn out and preheating: 60 min. at 850 °C
Program (Dekema)		Place investment ring directly into the pressing furnace from the preheating furnace (650/850 °C).	
Pressing furnace dwell time		L9 C650 T300	L9 C650 T300
Program for cooling investment ring		L9 C650 V.C385 VO T600	L9 C650 V.C390 VO T600
Positioning of the investment ring in the furnace	Opening downwards. Please make sure that the wax burn-out occurs outside of the investment ring, e.g.: – Tip out the investment ring in the direction of the rear wall – Support, e.g. with 3 small investment material cones (image)		
Preheating plunger	No	No	No
Preheating press blank	No	No	No
Important	No rapid cooling, as cracks may appear in the investment material. A change of preheating furnace (e.g. 650 °C to 390 °C) can also cause cracks.	–	–
Recommendation	As the preheating process is time consuming, preheating overnight is recommended.	–	–


5.4.6 Pressing

 The internal temperature of the investment ring must be 390°C.
This will be the case after a one hour setting time after reaching the final temperature (depending upon the quantity of investment rings in the furnace).

 DEKEMA press-i-dent: The press furnace must be sufficiently preheated to avoid incomplete pressing due to the cooled investment ring. Suggestion: The outside of the combustion chamber is lukewarm.


Prepare plunger and correct quantity of press blanks.


Carefully remove the investment ring from the preheating furnace using pliers and set it on a refractory support.

 Wear gloves for heat protection.




Carefully place press blanks into investment ring.

 Up to 2 press blanks can be used per press channel.
With the Trixpress system from DEKEMA, it is possible to provide the investment ring with more than one press channel.

 In case of 2 pressing blanks, place sides with logos on top of each other!



Place plunger in the investment ring with the rubber seal face down.

 Keep the loading time to 1 minute maximum to keep the escaping heat loss as low as possible.




Program overview (Pektkon® ivory)


Manufacturer	Furnace		Program
DEKEMA	Austromat 654 press-i-dent	100g	L9 T20.C380 V0 T570 L92 T40 V.C250 L8 V.C200 C0 L0 T5
		200g	L9 T20.C385 V0 T780 L92 T40 V.C250 L8 V.C200 C0 L0 T5
		380g (Trixpress)	L9 T20.C395 V0 T1200 L92 T40 V.C250 L8 V.C200 C0 L0 T5
	Austromat 3001 press-i-dent	100g	L9 T20.C390 V0 T600 L92 T40 V.C250 L8 V.C200 C0 L0 T5
		200g	L9 T20.C395 V0 T1200 L92 T40 V.C250 L8 V.C200 C0 L0 T5
		380g (Trixpress)	L9 T20.C395 V0 T1200 L92 T40 V.C250 L8 V.C200 C0 L0 T5

Cooling cycle

After the end of press cycle, the combustion chamber is flooded with fresh air by vacuum until the temperature reaches 200°C.

Then remove the investment ring from the press furnace using pliers.

 Wear gloves for heat protection.

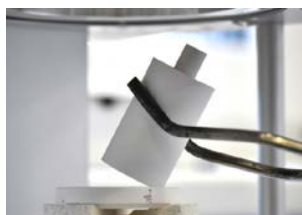



Cool the investment ring outside of the furnace to room temperature.



5.4.7 Divestment and cleaning


Using pliers, carefully remove the investment material without damaging the frames.

 Divest as soon as the investment ring is room temperature.

 Do not use tongs to divest larger pieces.




Fine divestment is carried out with abrasive 110 μ m aluminum oxide under pressure of 2 bars.

 Caution: Sandblast for a short period only to prevent damage.




Crown framework after fine divestment.

 The material can be pressed only one time.




5.5 Conditioning

 Cleaning with oil-free compressed air only.
Ceramic stones and old burs can cause clogging, which makes conditioning difficult and may lead to overlaps.

Check the fit and adjust, if necessary.




Cut the sprue by using a cutting wheel.

 When grinding the Pekkton® framework, wear protective goggles with a dust mask and use a suction unit.
The cutting wheels available from Cendres+Métaux SA are ideal for removing surplus material.



Cross-toothed milling is used to finish the framework.


 Speed limit maximum 15,000 rotations/min.
Do not work on the object if the pressure is too high.



Roughen the surface using a diamond milling cutter before sandblasting the framework.



After milling is complete, sandblast the framework with aluminum oxide 110 μ m under 2 bar pressure and clean well using oil-free compressed air.

 After sandblasting the surface, do not touch the surface with your bare fingers.
Never clean the framework with steam or water.




5.6 Veneering

5.6.1 Preparation

Before veneering, it is imperative that the Pekkton® framework is treated with composite primer.


We recommend the primer visio.link, Cendres+Métaux SA, Order No. 08000570.

 Please follow the manufacturer's instructions.




5.6.2 Veneering concepts

After preparation of the framework as described in Section 5.6.1, Pekkton® ivory can be refined esthetically in different ways. For example, it can be refined by veneering with composites, affixing custom-made pressable ceramic crowns or using prefabricated acrylic teeth and trays.

 As veneering is outside the area of responsibility of Cendres+Métaux SA, it is not further described in these instructions for use. Please follow the manufacturer's instructions for the veneering concept selected.

Information about the veneering concepts is available from our clinical case documentation on our website www.pekkton.com.

 Bridge work: To avoid cracks (and late effects) in the veneering as a result of different modulus of elasticity values for Pekkton® ivory and the veneering material, a separation should be made between the teeth down to the opaque.

5.7 Bond to titanium bases (laboratory)

The following procedure describes the cementation of titanium bases and frameworks of Pekkton® ivory.

In choosing cement, Multilink® Hybrid Abutment (Ivoclar Vivadent) is recommended.

1. The abutment is screwed onto the analog. Seal the screw channel of the titanium abutment and the Pekkton® ivory framework with wax.
2. Carefully sandblast the surface of the titanium abutment with 110µm aluminum oxide and 3 bar pressure.
3. Also carefully sandblast the contact surface on the inside of the framework. 110µm aluminum oxide and 2 bar pressure.
4. Monobond plus is applied to the sandblasted surfaces to silanize them. Application time approx. 60 seconds.
5. Apply visio.link (Bredent) to the Pekkton® ivory surface with a single-use brush and light cure for 90 seconds (Dentacolor XS, Kulzer).
6. Apply the cement to the inner surface of the framework and place on the abutment.
7. Then follow the manufacturer's instructions.

5.8 Try-in and cementation

5.8.1 Disinfection

After any fabrication or modification, the prosthetic work must be cleaned and disinfected according to national guidelines. When selecting the disinfectant, it is essential to ensure that:

- It is suitable for cleaning and disinfection of dental prosthetic components.
- It is compatible with the materials of the products to be cleaned and disinfected.
- It has tested efficacy in disinfection.

The prosthetic work must be disinfected with a high EPA-registered disinfectant prior to use. Recommended: Cidex® OPA Solution.

Strictly follow manufacturer's instructions.


5.8.2 Cementation


Preparation: (in the laboratory):

- 1) Sandblast the inner surface of the reconstruction with abrasive 110µm grit at a pressure of 2 bar.

Prior to cementation:

- 1) Check reconstruction for fit and correct by grinding, if necessary.
- 2) Occlusal precision corrections can be performed after cementation because composite veneering is very easy to polish in the patient's mouth.
- 3) Pretreat the inner surface with composite primer visio.link (Order No. 08000570) to increase the bond.

 Please follow the manufacturer's instructions for the visio.link.

 To increase the bond to Pekkton® ivory, the inner surface can be silicized before application of the composite primer and subsequently silanized.

Cementation:

Method of cementation:	Conventional (glass ionomer cements)	Self-adhesive	Adhesive
Stump	Length of stump > 4 mm Preparation angle: 4–8°	Length of stump > 4 mm Preparation angle: 4–8°	short stump, < 4 mm Preparation angle: > 8°

 Please follow the manufacturer's instructions.

5.9 Handling after integration





5.9.1 Cleaning and follow-up

It is best to clean your teeth and your dentures after every meal. Be careful when using tooth pastes. Do not use agents that are too abrasive. For further information, please contact your Cendres+ Métaux representative.

5.9.2 Traceability

The batch numbers must be documented to ensure traceability.

6 Ordering information

Material	Description	Order No.	Manufacturer
	Pekkton® ivory press blank (Core material)	0106 0003 (Packaging of 10 pieces)	Cendres+Métaux SA
	Disposable Pressplunger with seal (Diameter 12 mm)	0800 0141 (Packaging of 50 pieces)	Cendres+Métaux SA
		0800 0517 (Packaging of 3 pieces)	
	1 x 0106 0003 Pekkton® ivory press blanks (Packaging of 10 pieces) 3 x 0800 0517 Disposable Pressplunger with seal (Packaging of 3 pieces) and product information	0800 0518	Cendres+Métaux SA

7 Symbols

	Date of manufacture
	Manufacturer
	Patient No.
	Catalogue number
	Batch code
	Quantity
	Consult instructions for use
Rx only	Attention: According to US federal law, this product may only be sold by or on behalf of a physician.
	Cendres+Métaux SA products with CE labeling meet the requirements of the Medical Device Directive 93/42/EEC.
	
	Do not re-use
	Non-sterile
	Keep away from sunlight
	Attention (observe accompanying documents)

8 Disclaimer / Validity

The issuing of these instructions for use renders all previous versions invalid.

The manufacturer rejects any liability for damages resulting from non-compliance with these instructions for use.

In case of complaints, please always include the batch number.

Illustrated step-by-step instructions are available on the Cendres+Métaux homepage. www.cmsa.ch/dental

The product must be used exclusively by skilled persons.

9 Availability

Country-specific differences in product range are possible.

10 Copyright and trademarks

Pektkon® ivory is a registered trademark of Cendres+Métaux Holding SA, Biel/Bienne, Switzerland.

Reprints or publication – even excerpts – require the written permission of the publisher.

11 Further information

11.1 Troubleshooting

Problem	Cause	Solution
Workpiece not pressed out	<ul style="list-style-type: none"> – Investment ring has not been preheated to recommended temperature. – Investment ring too cold. – Duration of transport from the preheating furnace to the pressing furnace is too long. – Pressing furnace is too cold. – Insufficient material used. 	<ul style="list-style-type: none"> – Check program and final temperature. – Check calibration of the furnace. – Perform furnace change as quickly as possible. – Silver test. – Weigh press items before pressing.
Investment ring burst/broken	<ul style="list-style-type: none"> – Investment ring too cold. – Plunger is not properly inserted. – Dissimilar press items. – Minimum distance from the investment ring wall not maintained or too many items in too small an investment ring mold. 	<ul style="list-style-type: none"> – Check program and final temperature. – Make sure the plunger is not positioned at an angle in the investment ring channel. – Invest roughly same-size items (especially in the 100 g ring). – Take sufficient investment ring wall thickness into account. – Comply with the values stated.
Framework broke during divestment	<ul style="list-style-type: none"> – The divestment pliers got too close to the item, the margin. 	<ul style="list-style-type: none"> – Only divest roughly with the pliers, sandblast the rest.
Margins no longer fit properly after divestment	<ul style="list-style-type: none"> – Sandblasting pressure is too high. – Microbubbles. – Investment material residues on the inner surfaces. 	<ul style="list-style-type: none"> – Set max. pressure to 2 bar. – Fit carefully with a precision bur, then sandblast at 2 bar and 110 μm.
Veneer becomes detached from the framework (insufficient adhesion)	<ul style="list-style-type: none"> – Surface not properly prepared for bonding. – Primer not used. – Grease on the surface. – Moisture between the framework and the veneering material. 	<ul style="list-style-type: none"> – Prepare surface according to instructions. – Always use primer. – After sandblasting, never touch the surface with your fingers. – Do not clean the framework with water or steam.
Error message from the pressing furnace	Strictly follow the furnace manufacturer's operating instructions!	

11 FAQ

1 Can material be reused?

No. Too much effort would be involved in cleaning the material properly. Risk of impurity inclusions.

2 What composite veneering materials can I use?

Pekkton® ivory was successfully tested with various veneering composites, including SR Nexco (Ivoclar Vivadent), Gradia (GC), Ceramage (Shofu), VitaVM LC (Vita Zahnfabrik), Anaxblend and Anaxflow (Anaxdent), S.LAY (WEGOLD Edelmetalle) and Signum (Heraeus Kulzer).

3 If a bridge doesn't fit, can it be separated and rejoined?

No, this is not possible.

4 What is the situation regarding the formation of biofilm?

Results always depend on surface roughness. If surface quality is comparable, biofilm formation on high-performance polymers is less than on metal alloys, but slightly more than on ceramics.

5 What is the shrinkage of Pekkton® ivory?

≈ 1.3 % (volume).

6 How good is the precision?

The precision of single crowns is between 20µm and 50µm so it meets the clinical requirements of 50µm to 120µm maximum. However, precision always depends on how accurately the dental technician works.

7 What are the advantages over base metal restorations?

- Aesthetic, no black margins
- Metal-free
- No release of ions
- No taste of metal
- Non-conductive
- Corrosion-resistant
- Higher biocompatibility
- Less tool wear
- Easier polishing (5–10 times faster)
- Clean work (no dirt)
- Density 8 times lower
- Virtually insoluble

8 Regarding bridges, how many units are possible?

State of development today: With Pekkton® ivory, screw-retained bridges on implants (bonded to titanium bases) with maximum two pontics in the anterior and posterior region can be fabricated. Bridges on natural teeth with maximum one pontic.

9 Can the material be burred? When will bur blanks be available?

Pekkton® ivory is ideal for burring. The material is much quicker to machine than metals or ceramics so bur tool life can be considerably prolonged.

Pekkton® ivory is available as a milling rondel with 98.5mm diameter groove for CAD/CAM technology. Please note the information about availability and specification on our website www.pekkton.com